


# PatellarTape System™

## For Patellar Tendon Reconstruction

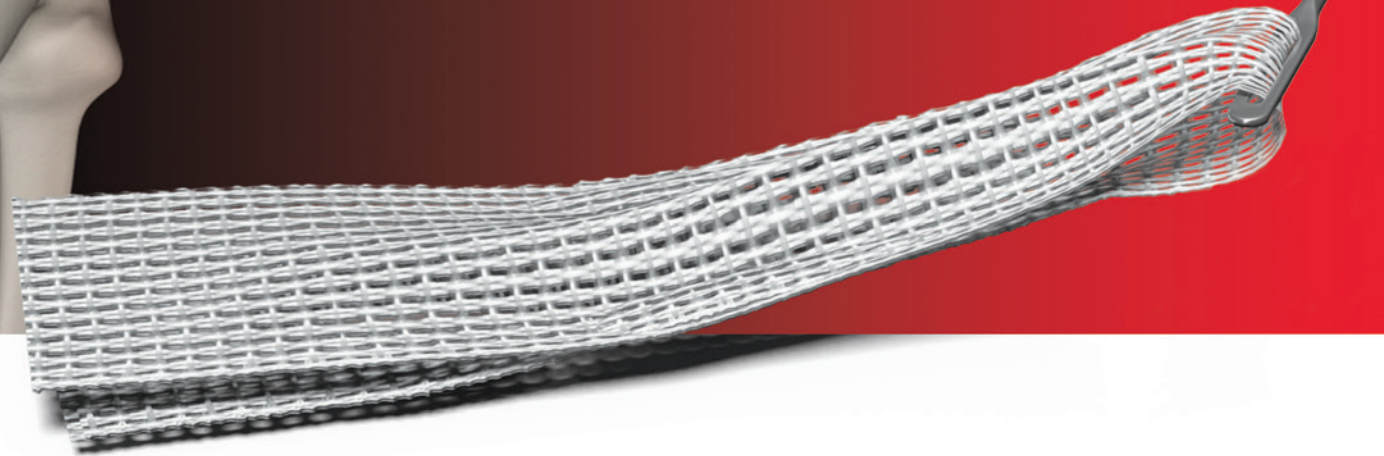

### Get involved

At Neoligaments we are constantly striving to improve outcomes for patients, and we want to hear from you.


Help us create the future of sports medicine and share your opinions and expertise with us at:

[www.neoligaments.com](http://www.neoligaments.com)

### Why PatellarTape System?

- Provides excellent intrinsic strength and allows early mobilization.
- The use of metalwork and wire cerclage is unnecessary and the associated high complication rate and problems of secondary removal are thus avoided.
- The implant carries none of the risks or availability problems of allograft.
- There is no donor site morbidity as encountered with autograft.
- It is a simple, easy to learn technique with a low complication rate.
- The open weave structure of the implant acts as a scaffold that encourages tissue ingrowth.



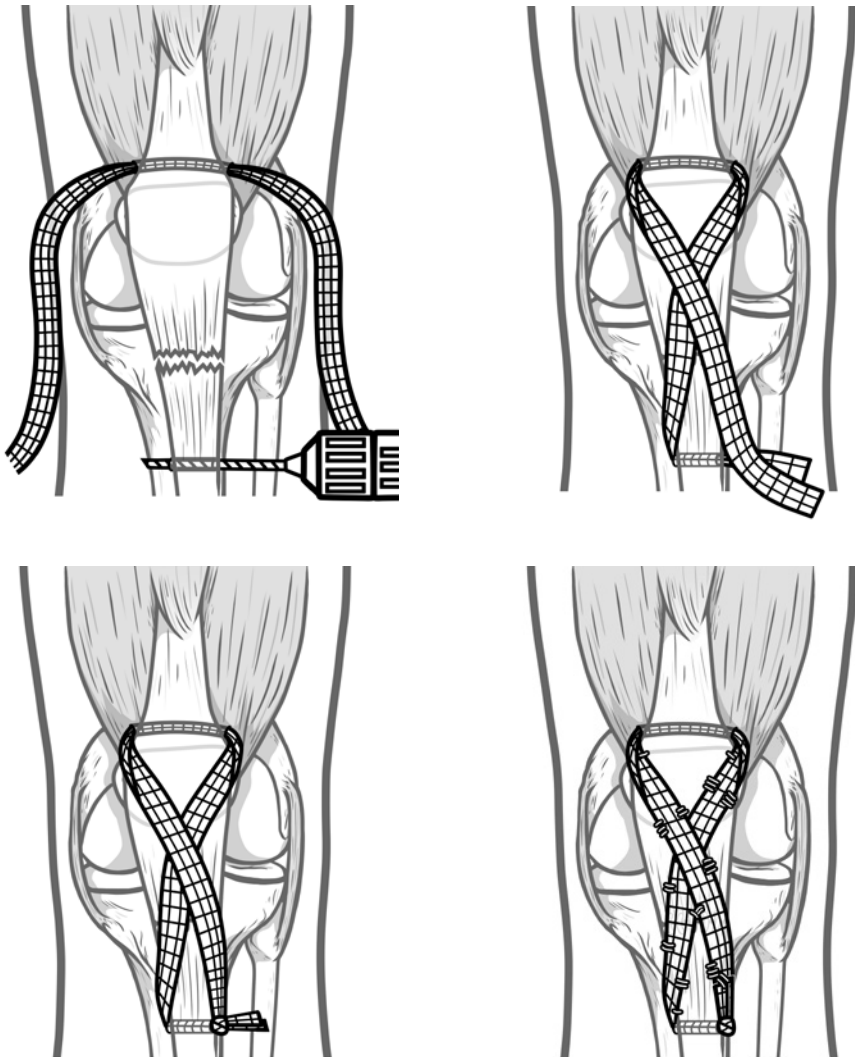

102-1062 PatellarTape System, includes:


Poly-Tape, 30 mm x 800 mm (supplied sterile)

Packaged with the following disposables:

Malleable probe with eye, stainless steel, 20 cm (supplied sterile)

Rigid probe with eye, stainless steel, 20 cm (supplied sterile)

Drill bit, plain shank to fit Jacobs Chuck, 4.5 mm diameter (supplied sterile)

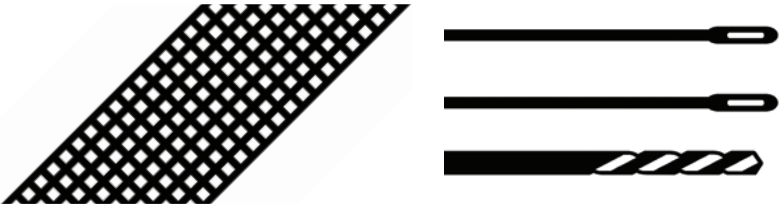

Optional Implant (dependent on method of fixation chosen by the user):

102-1381 Fastlok™, 8 mm x 23 mm (supplied sterile)

Fastlok Instruments:

202-1137 Impactor Assembly (non-sterile)

202-1118 Sliding Hammer (non-sterile)

Contact our Customer Services Department for further details or visit our website at [www.neoligaments.com](http://www.neoligaments.com)

Developed and manufactured by Neoligaments™, A division of Xiros™  
Springfield House, Whitehouse Lane, Leeds LS19 7UE  
Tel. +44 (0) 113 238 7202 Fax. +44 (0) 113 238 7201  
enquiries@neoligaments.com  
www.neoligaments.com  
Xiros Limited, registered in England No. 1664824.

All rights reserved. © Neoligaments™ 2018 Worldwide patents and patents pending. PatellarTape System, Fastlok, Neoligaments and Xiros are trademarks of Xiros.

The information above MUST NOT be used to perform the surgical procedure. Always refer to the Instructions for Use LAB 248 which contains detailed information and essential warnings and precautions.